# Compatibility table – pipette tips

## Pipette tips with filter

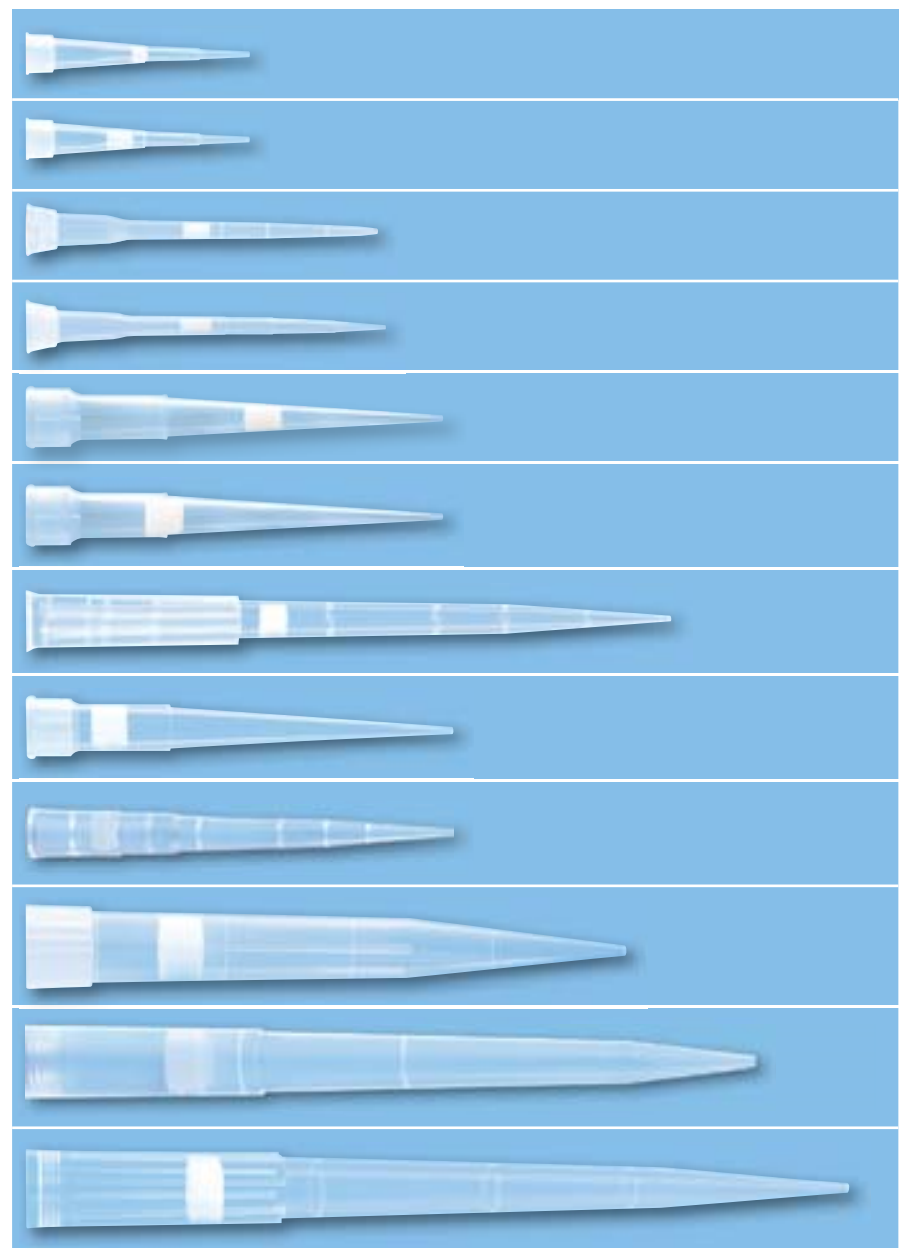

| Pipette tips with filter | Eppendorf® pipettes – Eppendorf Reference® | | | | | | | Eppendorf Research® | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 0.1-2.5 µl | 0.5-10 µl | 2-20 µl | 2-20 µl | 10-100 µl | 50-200 µl | 100-1,000 µl | 0.1-2.5 µl | 0.5-10 µl | 2-20 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 100-1,000 µl | 500-5,000 µl | 1-10 ml |
| 2.5 µl: 70.1130.212, 70.1130.217 | ● | ● 2.5 | ● 2.5 | | | | | ● | ● 2.5 | | | | | | | |
| 10 µl: 70.1130.210, 70.1130.215 | | ● | ● 10 | | | | | ✗ | ● | | | | | | | |
| 20 µl: 70.1114.210, 70.1114.215 | ● | ● | ● | | | | | ● | ● | | | | | | | |
| 20 µl: 70.1116.210, 70.1116.215 | ● | ● | ● | | | | | ● | ● | | | | | | | |
| 20 µl: 70.760.213, 70.760.219 | | | | ● | ● 20 | ● 20 | | | | ✗ | ● 20 | ● 20 | ✗ | | | |
| 100 µl: 70.760.212, 70.760.217 | | | | ● | ● | ● 100 | | | | ● | ● | ● 100 | ✗ | | | |
| 200 µl: 70.1189.215 | | | | ● | ● | ● | | | | ● | ● | ● | | | | |
| 200 µl: 70.760.211, 70.760.216 | | | | ✗ | ✗ | ● | | | | ✗ | ✗ | ● | ✗ | | | |
| 300 µl: 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | | ✗ | ✗ | ● | | | | ✗ | ✗ | ● | ● | | | |
| 1,000 µl: 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | | | | | ● | | | | | | | ● | | |
| 1,000 µl: 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | | | | | ● | | | | | | | ● | | |
| 1,250 µl: 70.1186.210, 70.1186.410 | | | | | | | ● | | | | | | | ● | | |

| Pipette tips with filter | Eppendorf® pipettes – Eppendorf Research® plus | | | | | | | | | | Eppendorf Research® pro | | | | | | | | | Xplorer® |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 0.1-2.5 µl | 0.5-10 µl MC | 2-20 µl | 2-20 µl | 10-100 µl MC | 20-200 µl | 30-300 µl MC | 100-1,000 µl | 500-5,000 µl | 1-10 ml | 0.5-10 µl | 0.5-10 µl MC | 5-100 µl | 5-100 µl MC | 20-300 µl | 20-300 µl MC | 50-1,000 µl | 50-1,200 µl MC | 100-5,000 µl | 0.5-10 µl MC |
| 2.5 µl: 70.1130.212, 70.1130.217 | ● | ● 2.5 | ● 2.5 | | | | | | | | ● 2.5 | ● 2.5 | | | | | | | | |
| 10 µl: 70.1130.210, 70.1130.215 | ✗ | ● | ● 10 | | | | | | | | ● | ● | | | | | | | | ● |
| 20 µl: 70.1114.210, 70.1114.215 | ● | ● | ● | | | | | | | | ● | ● | | | | | | | | ● |
| 20 µl: 70.1116.210, 70.1116.215 | ● | ● | ● | | | | | | | | ● | ● | | | | | | | | ● |
| 20 µl: 70.760.213, 70.760.219 | | | | ● | ● 20 | ● | ✗ | | | | | | ● 20 | ● 20 | | | | | | |
| 100 µl: 70.760.212, 70.760.217 | | | | ● | ● | ● 100 | ✗ | | | | | | ● | ● | | | | | | |
| 200 µl: 70.1189.215 | | | | ● | ● | ● | | | | | | | ● | | | | | | | |
| 200 µl: 70.760.211, 70.760.216 | | | | ✗ | ✗ | ● | ✗ | | | | | | | | ● 200 | ● 200 | | | | |
| 300 µl: 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | | | | ● | ● | | | | | | | | ● | ● | | | | |
| 1,000 µl: 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | | | | | | ● | | | | | | | | | ● | ✗ | | |
| 1,000 µl: 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | | | | | | ● | | | | | | | | | ● | | | |
| 1,250 µl: 70.1186.210, 70.1186.410 | | | | | | | | ● | | | | | | | | | ● | ● | | |

| Pipette tips with filter | Thermo® Finnpipettes – Finnpipette® Digital / F1 / F2 | | | | | | | | | | | | Finnpipette® Focus | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 0.2-2 µl | F2 0.5-5 µl | F1 1-10 µl | 0.5-10 µl Univ. | 0.5-10 µl MC | 2-20 µl Univ. | 5-50 µl MC | 10-100 µl Univ. | 20-200 µl Univ. | 50-300 µl MC | 100-1,000 µl | 200-1,000 µl | 0.3-3 µl | 0.5-5 µl | 1-10 µl | 30-300 µl | 100-1,000 µl |
| 2.5 µl: 70.1130.212, 70.1130.217 | ● | | | ● 2.5 | ● 2.5 | | | | | | | | ● | ● 2.5 | ● 2.5 | | |
| 10 µl: 70.1130.210, 70.1130.215 | | | | ● | ● | | | | | | | | | ● | ● | | |
| 20 µl: 70.1114.210, 70.1114.215 | ● | | ● | ● | ● | | | | | | | | | ● | ● | | |
| 20 µl: 70.1116.210, 70.1116.215 | ● | | | ● | ● | | | | | | | | | ● | ● | | |
| 20 µl: 70.760.213, 70.760.219 | | | | | | ● | | | ● 20 | | | | | | | ✗ | |
| 100 µl: 70.760.212, 70.760.217 | | | | | | | | ● | ● 100 | ● 100 | | | | | | ✗ | |
| 200 µl: 70.1189.215 | | | | | | ● | | ● | ● | | | | | | | | |
| 200 µl: 70.760.211, 70.760.216 | | | | | | ✗ | | ✗ | ● | | | | | | | ● 200 | |
| 300 µl: 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | | | | ✗ | | ✗ | ● | ● | | | | | | ● | |
| 1,000 µl: 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | | | | | | | | | ● | ● | | | | | ● |
| 1,000 µl: 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | | | | | | | | | ● | ● | | | | | ● |
| 1,250 µl: 70.1186.210, 70.1186.410 | | | | | | | | | | | ● | ● | | | | | ● |

| Pipette tips with filter | Finnpipette® Novus | | | | Bio Control | Gilson® pipettes – Pipetman® / Ultra / Concept | | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 30-300 µl | 30-300 µl MC | 100-1,000 µl | 100-1,200 µl MC | 50-300 µl MC | P2/U2 0.2-2 µl | P10/U10 0,1-10 µl | C8/C12 1-10 µl | P20/U20 2-20 µl | P100/U100 20-100 µl | P200/U200 20-200 µl | U8 20-300 µl | P1,000/U3,000 200-1,000 µl | P5,000/U5,000 1,000-5,000 µl | P10/U10 1-10 ml |
| 2.5 µl: 70.1130.212, 70.1130.217 | | | | | | ● | ● 2.5 | ✗ | | | | | | | |
| 10 µl: 70.1130.210, 70.1130.215 | | | | | | ● | ● | ✗ | | | | | | | |
| 20 µl: 70.1114.210, 70.1114.215 | | | | | | ● | ✗ | | | | | | | | |
| 20 µl: 70.1116.210, 70.1116.215 | | | | | | ● | ● | ✗ | | | | | | | |
| 20 µl: 70.760.213, 70.760.219 | | | | | | | | | ● | ● 20 | | | | | |
| 100 µl: 70.760.212, 70.760.217 | | | | | | | | | ✗ | ● | ● | | | | |
| 200 µl: 70.1189.215 | | | | | | | | | ● | ● | ● | | | | |
| 200 µl: 70.760.211, 70.760.216 | ● 200 | ● 200 | | | | | | | ✗ | ✗ | ● | ✗ | | | |
| 300 µl: 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | | | ● | | | | ✗ | ✗ | ● | ● | | | |
| 1,000 µl: 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | ● | | | | | | | | | | ● | | |
| 1,000 µl: 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | ● | | | | | | | | | | ● | | |
| 1,250 µl: 70.1186.210, 70.1186.410 | | | | ● | | | | | | | | | ● | | |

## Pipette tips without filter

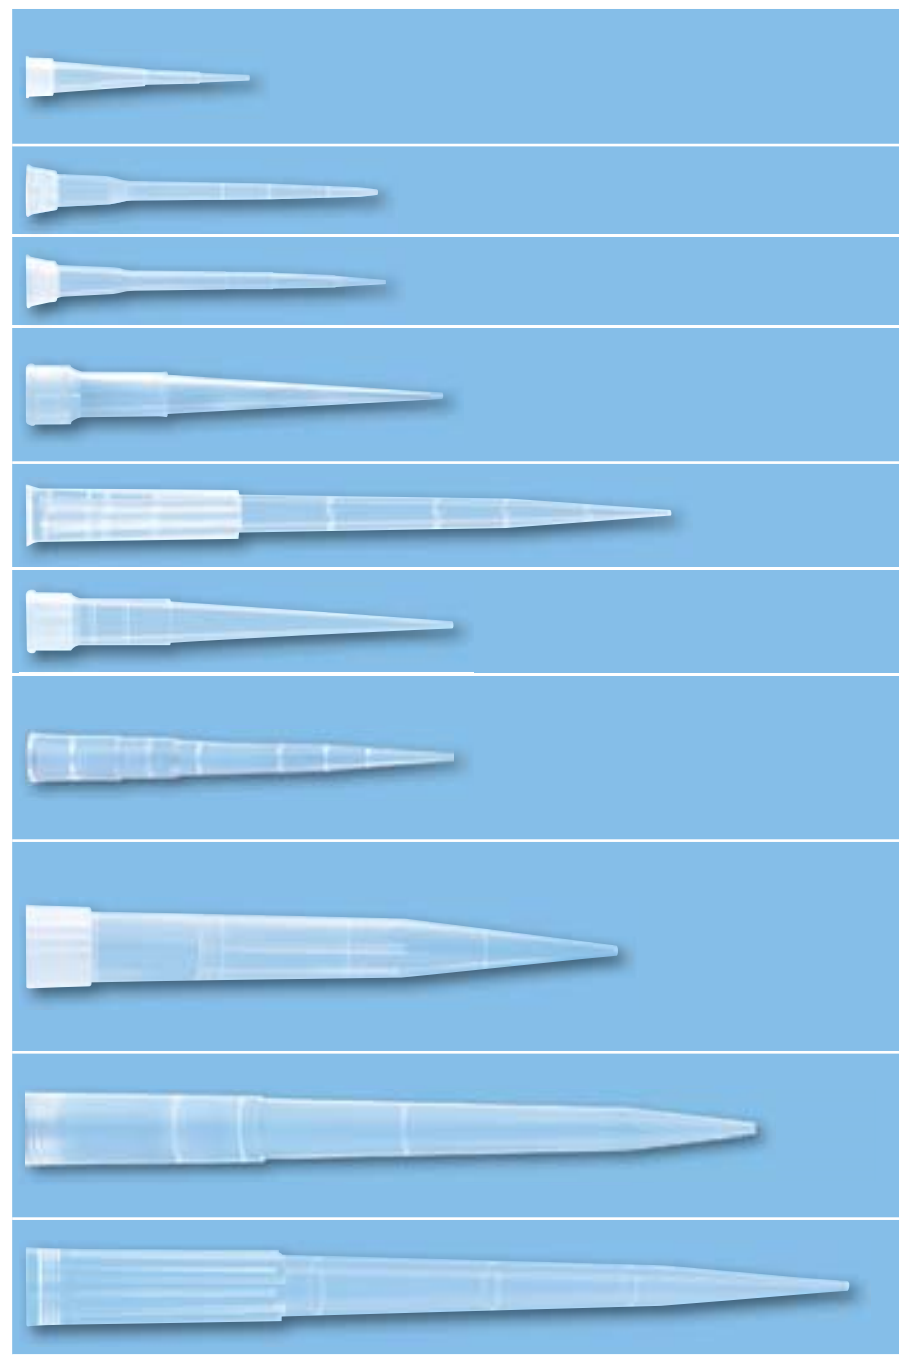

| Pipette tips without filter | Eppendorf Reference® | | | | | | | Eppendorf Research® | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 0.1-2.5 µl | 0.5-10 µl | 2-20 µl | 2-20 µl | 10-100 µl | 50-200 µl | 100-1,000 µl | 0.1-2.5 µl | 0.5-10 µl | 2-20 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 100-1,000 µl | 500-5,000 µl | 1-10 ml |
| 10 µl: 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | ● | ● | ● | | | | | ● | ● | | | | | | | |
| 20 µl: 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | ● | ● | ● | | | | | ✗ | ● | | | | | | | |
| 20 µl: 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | ● | ● | ● | | | | | ● | ● | | | | | | | |
| 200 µl: 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | | ● | ● | ● | | | | ● | ● | ● | ✗ | | | |
| 200 µl: 70.1189.105 | | | | ● | ● | ● | | | | ● | ● | ● | | | | |
| 250 µl: 70.3031, 70.760.201, 70.760.501 | | | | ● | ● | ● | | | | | | ● | ✗ | | | |
| 300 µl: 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | | | | ✗ | ✗ | ● | | | | ✗ | ✗ | ● | ● | | | |
| 1,000 µl: 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | | | | | ● | | | | | | | ● | | |
| 1,250 µl: 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | | | | | ● | | | | | | | ● | | |
| 1,250 µl: 70.1186, 70.1186.100, 70.1186.200 | | | | | | | ● | | | | | | | ● | | |

| Pipette tips without filter | Eppendorf Research® plus | | | | | | | | | | Eppendorf Research® pro | | | | | | | | | Xplorer® |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 0.1-2.5 µl | 0.5-10 µl MC | 2-20 µl | 2-20 µl | 10-100 µl MC | 20-200 µl | 30-300 µl MC | 100-1,000 µl | 500-5,000 µl | 1-10 ml | 0.5-10 µl | 0.5-10 µl MC | 5-100 µl | 5-100 µl MC | 20-300 µl | 20-300 µl MC | 50-1,000 µl | 50-1,200 µl MC | 100-5,000 µl | 0.5-10 µl MC |
| 10 µl: 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | ● | ● | ● 10 | | | | | | | | ● | ● | | | | | | | | ● |
| 20 µl: 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | ● | ● | ● | | | | | | | | ● | ● | | | | | | | | ● |
| 20 µl: 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | ● | ● | ● | | | | | | | | ● | ● | | | | | | | | ● |
| 200 µl: 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | | ● | ● | ● | ✗ | | | | | | ● | ● | | | | | | |
| 200 µl: 70.1189.105 | | | | ● | ● | ● | | | | | | | ● | | | | | | | |
| 250 µl: 70.3031, 70.760.201, 70.760.501 | | | | | ● | ● | ✗ | | | | | | | | ● 250 | ● 250 | | | | |
| 300 µl: 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | | | | ✗ | ✗ | ● | ● | | | | | | ✗ | ✗ | ● | ● | | | | |
| 1,000 µl: 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | | | | | | ● | | | | | | | | | ● | ✗ | | |
| 1,250 µl: 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | | | | | | ● | | | | | | | | | ● | | | |
| 1,250 µl: 70.1186, 70.1186.100, 70.1186.200 | | | | | | | | ● | | | | | | | | | ● | ● | | |

| Pipette tips without filter | Finnpipette® Digital / F1 / F2 | | | | | | | | | | | | Finnpipette® Focus | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 0.2-2 µl | F2 0.5-5 µl | F1 1-10 µl | 0.5-10 µl Univ. | 0.5-10 µl MC | 2-20 µl Univ. | 5-50 µl MC | 10-100 µl Univ. | 20-200 µl Univ. | 50-300 µl MC | 100-1,000 µl | 200-1,000 µl | 0.3-3 µl | 0.5-5 µl | 1-10 µl | 30-300 µl | 100-1,000 µl |
| 10 µl: 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | ● | | | ● | ● | | | | | | | | ● | ● | ● | | |
| 20 µl: 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | ● | ● | ● | ● | ● | | | | | | | | | ● | ● | | |
| 20 µl: 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | ● | | | ● | ● | | | | | | | | | ● | ● | | |
| 200 µl: 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | | | | ● | | ● | ● | ● 200 | | | | | | ✗ | |
| 200 µl: 70.1189.105 | | | | | | ● | | ● | ● | | | | | | | | |
| 250 µl: 70.3031, 70.760.201, 70.760.501 | | | | | | ✗ | | ✗ | ● | | | | | | | ● 250 | |
| 300 µl: 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | | | | | | ✗ | | ✗ | ● | ● | | | | | | ● | |
| 1,000 µl: 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | | | | | | | | | ● | ● | | | | | ● |
| 1,250 µl: 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | | | | | | | | | ● | ● | | | | | ● |
| 1,250 µl: 70.1186, 70.1186.100, 70.1186.200 | | | | | | | | | | | ● | ● | | | | | ● |

| Pipette tips without filter | Finnpipette® Novus | | | | Bio Control | Pipetman® / Ultra / Concept | | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | 30-300 µl | 30-300 µl MC | 100-1,000 µl | 100-1,200 µl MC | 50-300 µl MC | P2/U2 0.2-2 µl | P10/U10 0,1-10 µl | C8/C12 1-10 µl | P20/U20 2-20 µl | P100/U100 20-100 µl | P200/U200 20-200 µl | U8 20-300 µl | P1,000/U3,000 200-1,000 µl | P5,000/U5,000 1,000-5,000 µl | P10/U10 1-10 ml |
| 10 µl: 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | | | | | | ● | ● | ✗ | | | | | | | |
| 20 µl: 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | | | | | | ● | ✗ | | | | | | | | |
| 20 µl: 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | | | | | | ● | ● | ✗ | | | | | | | |
| 200 µl: 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | | | | | | | ● | ● | ● | ● 200 | | | |
| 200 µl: 70.1189.105 | | | | | | | | | ● | ● | ● | | | | |
| 250 µl: 70.3031, 70.760.201, 70.760.501 | | | | | | | | | ✗ | ✗ | ● | ● 250 | | | |
| 300 µl: 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | ● | ● | | | ● | | | | ✗ | ✗ | ● | ● | | | |
| 1,000 µl: 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | ● | ✗ | | | | | | | | | ● | | |
| 1,250 µl: 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | ● | | | | | | | | | | ● | | |
| 1,250 µl: 70.1186, 70.1186.100, 70.1186.200 | | | | ● | | | | | | | | | ● | | |

● = compatible
10 = reduced pipetting volume
✗ = not recommended

= not checked
MC = multi-channel pipette

Pipette manufacturers revise or modify the pipette cones on their pipettes as part of technical changes. Our recommendations in the compatibility table can therefore only be taken as a guide. In case of doubt, we are happy to provide sample tips to you free of charge in order to ensure the optimal fit and performance of our tips with your pipettes.

Technical modifications reserved
This document may contain information on products that may not be available in particular countries

25_809_0200_503

SARSTEDT

# Compatibility table – pipette tips

## Biohit-Sartorius® pipettes

### Pipette tips with filter

| | | mLine® Mechanical | | | | | | | | Proline® Mechanical | | | | | | | | | eLine® Electronic | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Volume | Article no. | 0.5-10 µl | 0.5-10 µl MC | 2-20 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 100-1,000 µl | 100-5,000 µl | 0.1-2.5 µl | 0.5-10 µl | 5-50 µl | 5-50 µl MC | 20-200 µl | 50-250 µl MC | 50-300 µl MC | 100-1,000 µl | 100-5,000 µl | 0.2-10 µl | 10-300 µl | 50-1,000 µl | 50-1,200 µl MC | 100-5,000 µl |
| 2.5 µl | 70.1130.212, 70.1130.217 | ● 2.5 | ● 2.5 | | | | | | | ● | ● 2.5 | | | | | | | | ● 2.5 | | | | |
| 10 µl | 70.1130.210, 70.1130.215 | ● | ● | | | | | | | | ● | | | | | | | | ● | | | | |
| 20 µl | 70.1114.210, 70.1114.215 | ● | | | | | | | | | | | | | | | | | | | | | |
| 20 µl | 70.1116.210, 70.1116.215 | ● | ● | | | | | | | ● | ● | | | | | | | | ● | | | | |
| 20 µl | 70.760.213, 70.760.219 | | | | ✗ | ✗ | ✗ | | | | | ● 20 | ● 20 | ✗ | ✗ | ✗ | | | | ✗ | | | |
| 100 µl | 70.760.212, 70.760.217 | | | | ✗ | ● 100 | | | | | | ● | ● | ● 100 | ✗ | ✗ | | | | ✗ | | | |
| 200 µl | 70.1189.215 | | | ● | ● | ● | | | | | | ● | | ● | | | | | | | | | |
| 200 µl | 70.760.211, 70.760.216 | | | | ✗ | ● | | | | | | ✗ | ✗ | ● | ● 200 | ● 200 | | | | ✗ | | | |
| 300 µl | 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | | ✗ | ● | ● | | | | | ✗ | ✗ | ● | ● | ● | | | | ● | | | |
| 1,000 µl | 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | | | | | ● | | | | | | | | | ● | | | | ● | ✗ | |
| 1,000 µl | 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | | | | | ● | | | | | | | | | ● | | | | ● | | |
| 1,250 µl | 70.1186.210, 70.1186.410 | | | | | | | ● | | | | | | | | | ● | | | | | ✗ | |

### Pipette tips without filter

| | | mLine® Mechanical | | | | | | | | Proline® Mechanical | | | | | | | | | eLine® Electronic | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Volume | Article no. | 0.5-10 µl | 0.5-10 µl MC | 2-20 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 100-1,000 µl | 100-5,000 µl | 0.1-2.5 µl | 0.5-10 µl | 5-50 µl | 5-50 µl MC | 20-200 µl | 50-250 µl MC | 50-300 µl MC | 100-1,000 µl | 100-5,000 µl | 0.2-10 µl | 10-300 µl | 50-1,000 µl | 50-1,200 µl MC | 100-5,000 µl |
| 10 µl | 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | ● | ● | | | | | | | ● | ● | | | | | | | | ● | | | | |
| 20 µl | 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | ● | | | | | | | | | | | | | | | | | | | | | |
| 20 µl | 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | ● | ● | | | | | | | ● | ● | | | | | | | | ● | | | | |
| 200 µl | 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | | ✗ | ● | ✗ | | | | | ● | ● | ✗ | ✗ | ✗ | | | | ✗ | | | |
| 200 µl | 70.1189.105 | | | ● | ● | ● | | | | | | ● | | ● | | | | | | | | | |
| 250 µl | 70.3031, 70.760.201, 70.760.501 | | | | ✗ | ● | | | | | | ● | ● | ● | ● | ● 250 | | | | ✗ | | | |
| 300 µl | 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | | | | ✗ | ● | ● | | | | | ✗ | ✗ | ● | ● | ● | | | | ● | | | |
| 1,000 µl | 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | | | | | ● | | | | | | | | | ● | | | | ● | ✗ | |
| 1,250 µl | 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | | | | | ● | | | | | | | | | ● | | | | ● | | |
| 1,250 µl | 70.1186, 70.1186.100, 70.1186.200 | | | | | | | ● | | | | | | | | | ● | | | | | ✗ | |

## Brand® pipettes

### Pipette tips with filter

| | | Transferpette® Digital | | | | | | | | | | Transferpette® S | | | | | | | | | Transferpette® Electronic | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Volume | Article no. | 0.1-1 µl | 0.5-10 µl | 2-20 µl | 2-20 µl | 5-50 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 25-250 µl | 100-1,000 µl | 0.1-1 µl | 0.5-10 µl | 0.5-10 µl MC | 2-20 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 100-1.000 µl | 1-10 ml | 0.5-10 µl | 0.5-10 µl MC | 2-20 µl | 1-20 µl MC | 20-200 µl | 100-1,000 µl |
| 2.5 µl | 70.1130.212, 70.1130.217 | ✗ | ● 2.5 | ● 2.,5 | | | | | | | | ✗ | ● 2.5 | ● 2.5 | | | | | | | ● 2.5 | ● 2.5 | ● 2.5 | ● 2.5 | | |
| 10 µl | 70.1130.210, 70.1130.215 | ✗ | ● | ● 10 | | | | | | | | ✗ | ● | ● | | | | | | | ● | ● | ● | ● | | |
| 20 µl | 70.1114.210, 70.1114.215 | | ● | ● | | | | | | | | ✗ | | | | | | | | | | | | | | |
| 20 µl | 70.1116.210, 70.1116.215 | ✗ | ● | ● | | | | | | | | ✗ | ● | ● | | | | | | | ● | ● | ● | ● | | |
| 20 µl | 70.760.213, 70.760.219 | | | | ● | ● | ● 20 | ✗ | ✗ | | | | | | ● | ● 20 | ● 20 | ✗ | | | | | | | ● 20 | |
| 100 µl | 70.760.212, 70.760.217 | | | | ✗ | ✗ | ✗ | ✗ | ✗ | | | | | | ✗ | ✗ | ● 100 | ✗ | | | | | | | ● 100 | |
| 200 µl | 70.1189.215 | | | | | | | | | | | | | | | | | | | | | | | | | |
| 200 µl | 70.760.211, 70.760.216 | | | | ✗ | ✗ | ✗ | ✗ | ✗ | | | | | | ✗ | ✗ | ● | ✗ | | | | | | | ● 100 | |
| 300 µl | 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | | ✗ | ✗ | ✗ | ● | ● | | | | | | ✗ | ✗ | ● | ✗ | | | | | | | ● | |
| 1,000 µl | 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | | | | | | | ✗ | ● | | | | | | | | ● | | | | | | | ● |
| 1,000 µl | 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | | | | | | | | ● | | | | | | | | ● | | | | | | | ● |
| 1,250 µl | 70.1186.210, 70.1186.410 | | | | | | | | | ✗ | ● | | | | | | | | ● | | | | | | | ● |

### Pipette tips without filter

| | | Transferpette® Digital | | | | | | | | | | Transferpette® S | | | | | | | | | Transferpette® Electronic | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Volume | Article no. | 0.1-1 µl | 0.5-10 µl | 2-20 µl | 2-20 µl | 5-50 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 25-250 µl | 100-1,000 µl | 0.1-1 µl | 0.5-10 µl | 0.5-10 µl MC | 2-20 µl | 10-100 µl | 20-200 µl | 30-300 µl MC | 100-1.000 µl | 1-10 ml | 0.5-10 µl | 0.5-10 µl MC | 2-20 µl | 1-20 µl MC | 20-200 µl | 100-1,000 µl |
| 10 µl | 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | ● | ● | ● | | | | | | | | ✗ | ● | ● | | | | | | | ● | ● | ● | ● | | |
| 20 µl | 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | | ● | ● | | | | | | | | | | | | | | | | | | | | | | |
| 20 µl | 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | ✗ | ● | ● | | | | | | | | ✗ | ● | ● | | | | | | | ● | ● | ● | ● | | |
| 200 µl | 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | | ● | ● | ● | ✗ | ✗ | | | | | | ● | ● | ● | ✗ | | | | | | | ● | |
| 200 µl | 70.1189.105 | | | | | | | | | | | | | | | | | | | | | | | | | |
| 250 µl | 70.3031, 70.760.201, 70.760.501 | | | | ● | ● | ● | ✗ | ✗ | | | | | | ● | ● | ● | ✗ | | | | | | | ● | |
| 300 µl | 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | | | | ✗ | ✗ | ✗ | ● | ● | | | | | | ✗ | ✗ | ● | ✗ | | | | | | | ● | |
| 1,000 µl | 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | | | | | | | ● | ● | | | | | | | | ● | | | | | | | ● |
| 1,250 µl | 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | | | | | | | ● | ● | | | | | | | | ● | | | | | | | ● |
| 1,250 µl | 70.1186, 70.1186.100, 70.1186.200 | | | | | | | | | ● | ● | | | | | | | | ● | | | | | | | ● |

## Socorex® manual/electronic pipettes

### Pipette tips with filter

| | | Calibra® Manual Micro 822 | | | | | | | C. M. Multi 852 | | | Acura® Manual Micro 825 / Acura® Electro Micro 925 | | | | | | | | A. 835/935e | Acura® Multi 855/955e | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Volume | Article no. | 0.2-2 µl | 1-10 µl | 1-10 µl | 2-20 µl | 10-100 µl | 20-200 µl | 100-1,000 µl | 1-10 µl | 10-100 µl | 20-200 µl | 0.1-2 µl | 0.5-10 µl | 1-10 µl | 2-20 µl | 5-50 µl | 10-100 µl | 10-200 µl | 100-1,000 µl | 0.5-5 ml | 0.5-10 µl MC | 5-50 µl MC | 20-200 µl MC |
| 2.5 µl | 70.1130.212, 70.1130.217 | ● | ● 2.5 | | | | | | ● 2.5 | | | ● | ✗ | | | | | | | | ● 2.5 | | |
| 10 µl | 70.1130.210, 70.1130.215 | ● | ● | | | | | | ● | | | ● | ● | | | | | | | | ● | | |
| 20 µl | 70.1114.210, 70.1114.215 | ● | ● | | | | | | | | | ● | ● | | | | | | | | | | |
| 20 µl | 70.1116.210, 70.1116.215 | ✗ | ✗ | | | | | | ✗ | | | ● | ● | | | | | | | | | | |
| 20 µl | 70.760.213, 70.760.219 | | | ● 10 | ● | ● 20 | ✗ | | | ● | ✗ | | | ● | ● | ● 20 | ● 20 | ✗ | | | | ● | ✗ |
| 100 µl | 70.760.212, 70.760.217 | | | ✗ | ✗ | ✗ | ● 100 | | | ✗ | ● | | | ✗ | ✗ | ● | ● | ● 100 | | | | ● | ● 100 |
| 200 µl | 70.1189.215 | | | | | | | | | | | | | | ● | ● | ● | ● | | | | | |
| 200 µl | 70.760.211, 70.760.216 | | | ✗ | ✗ | ✗ | ✗ | | | ✗ | ✗ | | | ✗ | ✗ | ✗ | ✗ | ● | | | | ✗ | ● |
| 300 µl | 70.3040.255, 70.3040.275, 70.3040.355, 70.3040.375 | | | ✗ | ✗ | ✗ | ● | | | ✗ | ✗ | | | ✗ | ✗ | ✗ | ✗ | ● | | | | ✗ | ● |
| 1,000 µl | 70.3050.255, 70.3050.275, 70.3050.355, 70.3050.375 | | | | | | | ● | | | | | | | | | | | ● | | | | |
| 1,000 µl | 70.3060.255, 70.3060.275, 70.3060.355, 70.3060.375 | | | | | | | ● | | | | | | | | | | | ● | | | | |
| 1,250 µl | 70.1186.210, 70.1186.410 | | | | | | | ● | | | | | | | | | | | ● | | | | |

### Pipette tips without filter

| | | Calibra® Manual Micro 822 | | | | | | | C. M. Multi 852 | | | Acura® Manual Micro 825 / Acura® Electro Micro 925 | | | | | | | | A. 835/935e | Acura® Multi 855/955e | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Volume | Article no. | 0.2-2 µl | 1-10 µl | 1-10 µl | 2-20 µl | 10-100 µl | 20-200 µl | 100-1,000 µl | 1-10 µl | 10-100 µl | 20-200 µl | 0.1-2 µl | 0.5-10 µl | 1-10 µl | 2-20 µl | 5-50 µl | 10-100 µl | 10-200 µl | 100-1,000 µl | 0.5-5 ml | 0.5-10 µl MC | 5-50 µl MC | 20-200 µl MC |
| 10 µl | 70.3010, 70.1130.100, 70.1130.105, 70.1130.200, 70.1130.600 | ● | ● | | | | | | ● | | | ● | ● | | | | | | | | ● | | |
| 20 µl | 70.3020, 70.1114.100, 70.1114.105, 70.1114.200 | ● | ● | | | | | | | | | ● | ● | | | | | | | | | | |
| 20 µl | 70.3021, 70.1116.100, 70.1116.105, 70.1116.200 | ● | ● | | | | | | ✗ | | | ● | ● | | | | | | | | | | |
| 200 µl | 70.3030, 70.760.102, 70.760.107, 70.3030.020, 70.760.202, 70.760.502 | | | ● | ● | ● | ● | | | ● | ● | | | ● | ● | ● | ● | ● | | | | ● | ● |
| 200 µl | 70.1189.105 | | | | | | | | | | | | | | ● | ● | ● | ● | | | | | |
| 250 µl | 70.3031, 70.760.201, 70.760.501 | | | ✗ | ✗ | ✗ | ● | | | ✗ | ✗ | | | ✗ | ✗ | ✗ | ✗ | ● | | | | ✗ | ● |
| 300 µl | 70.3040, 70.3040.100, 70.3040.110, 70.3040.200, 70.3040.205, 70.3040.210, 70.3040.305 | | | ✗ | ✗ | ✗ | ● | | | ✗ | ✗ | | | ✗ | ✗ | ● | ● | ● | | | | ✗ | ● |
| 1,000 µl | 70.3050, 70.3050.020, 70.3050.030, 70.3050.100, 70.3050.110, 70.3050.200, 70.3050.205, 70.3050.210, 70.3050.305 | | | | | | | ● | | | | | | | | | | | ● | | | | |
| 1,250 µl | 70.3060, 70.3060.100, 70.3060.110, 70.3060.200, 70.3060.205, 70.3060.210, 70.3060.305 | | | | | | | ● | | | | | | | | | | | ● | | | | |
| 1,250 µl | 70.1186, 70.1186.100, 70.1186.200 | | | | | | | ● | | | | | | | | | | | ● | | | | |

● = compatible
10 = reduced pipetting volume
✗ = not recommended
(shaded) = not checked
MC = multi-channel pipette

Pipette manufacturers revise or modify the pipette cones on their pipettes as part of technical changes. Our recommendations in the compatibility table can therefore only be taken as a guide. In case of doubt, we are happy to provide sample tips to you free of charge in order to ensure the optimal fit and performance of our tips with your pipettes.

SARSTEDT